





Extracorporeal CO₂ removal system



- ➔ **Minimally invasive**
- ➔ **Effective**
- ➔ **Simple and safe**
- ➔ **Automated**

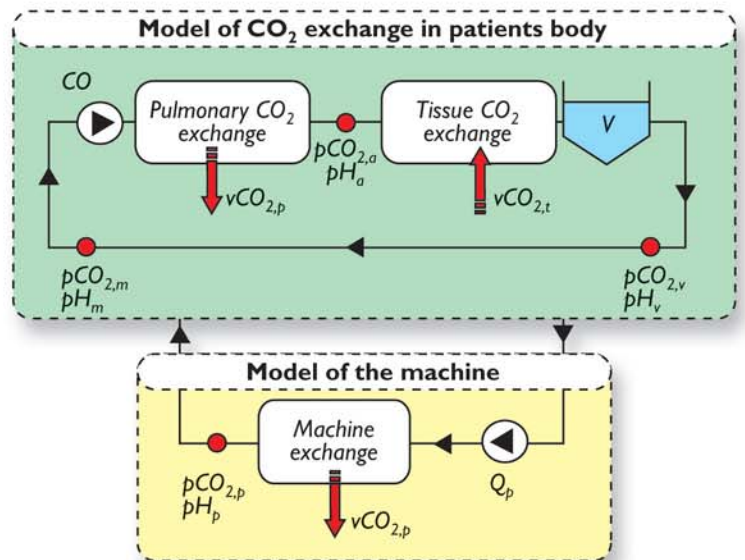

Pushes the boundaries of protective ventilation

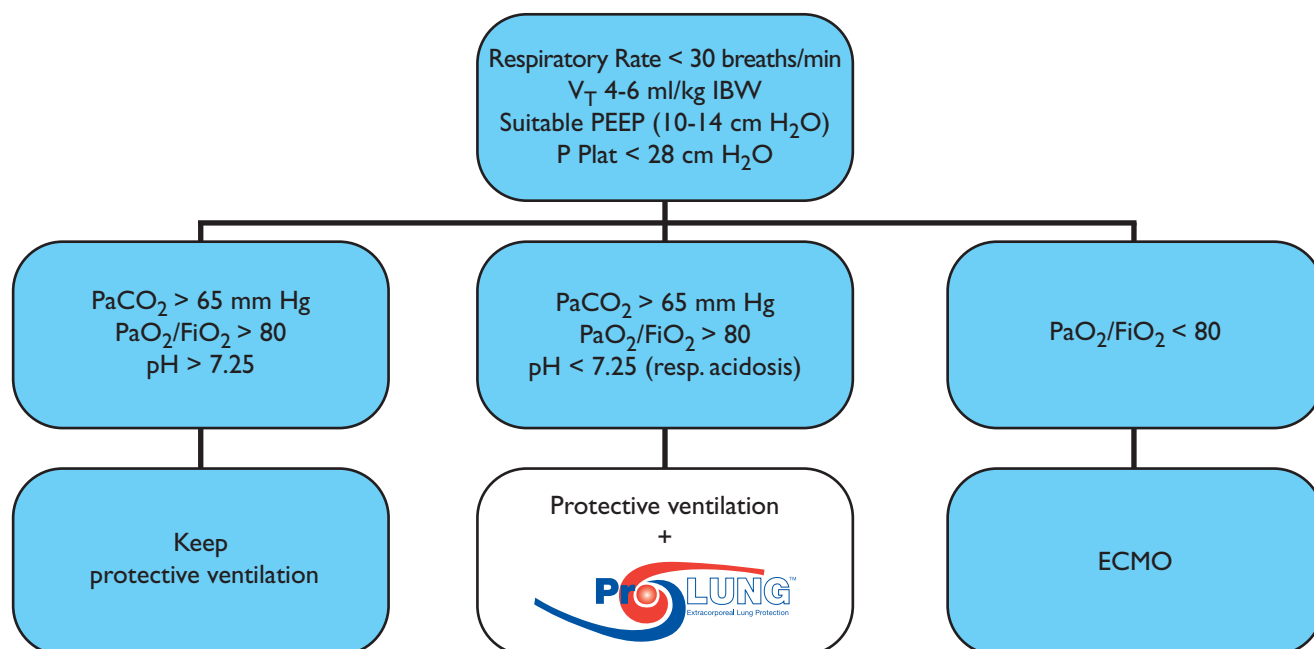

Bibliografia

- Gattinoni L, Pesenti A, Avalli L, Rossi F, Bombino M (1987) Pressure-volume curve of total respiratory system in acute respiratory failure. Computed tomographic scan study. *Am Rev Respir Dis* 136(3):730-6.
- Ranieri VM, Suter PM, Tortorella C, De Tullio R, Dayer JM, Brienza A, Bruno F, Slutsky AS (1999) Effect of mechanical ventilation on inflammatory mediators in patients with acute respiratory distress syndrome: a randomized controlled trial. *Jama* 282(1):54-61.
- Malhotra A (2007) Low-tidal-volume ventilation in the acute respiratory distress syndrome. *N Engl J Med* 357(11):1113-20.
- ARDS Network (2000) Ventilation with lower tidal volumes as compared with traditional tidal volumes for acute lung injury and the acute respiratory distress syndrome. *N Engl J Med* 342(18):1301-8.
- Hager DN, Krishnan JA, Hayden DL, Brower RG (2005) Tidal volume reduction in patients with acute lung injury when plateau pressures are not high. *Am J Respir Crit Care Med* 172(10):1241-5.
- Gattinoni L, Pesenti A, Mascheroni D, Marcolin R, Fumagalli R, Rossi F, Iapichino G, Romagnoli G, Uziel L, Agostoni A, et al. (1986) Low-frequency positive-pressure ventilation with extracorporeal CO₂ removal in severe acute respiratory failure. *Jama* 256(7):881-6.
- Hickling KG, Walsh J, Henderson S, Jackson R. Low mortality rate in adult respiratory distress syndrome using low-volume, pressure-limited ventilation with permissive hypercapnia: a prospective study. *Crit Care Med*. 1994 Oct;22(10):1568-78.
- Richard JC, Brochard L, Breton L, Aboab J, Vandelet P, Tamion F, Maggiore SM, Mercat A, Bonmarchand G. Influence of respiratory rate on gas trapping during low volume ventilation of patients with acute lung injury. *Intensive Care Med*. 2002 Aug;28(8):1078-83.

Code	Description
PLFLOW	ProLUNG hemoperfusion module
PLMETER	ProLUNG gas control unit
PLLUNGP	ProLUNG Kit for extracorporeal CO ₂ removal

ESTOR S.P.A.
Via Newton, 12 - 20016 Pero (MI)
Tel. +39 (0)2339416.1 - Fax +39 (0)233912069
estor@estor.it • www.estor.it

The trademark  is property of Estor S.P.A.

Distributed by

