


Yesterday's standard practice = Intra-op hypothermia


INTRA-OP HYPOTHERMIA

Typical Pattern of Hypothermia During General Anesthesia with Forced-Air Intraoperative Warming

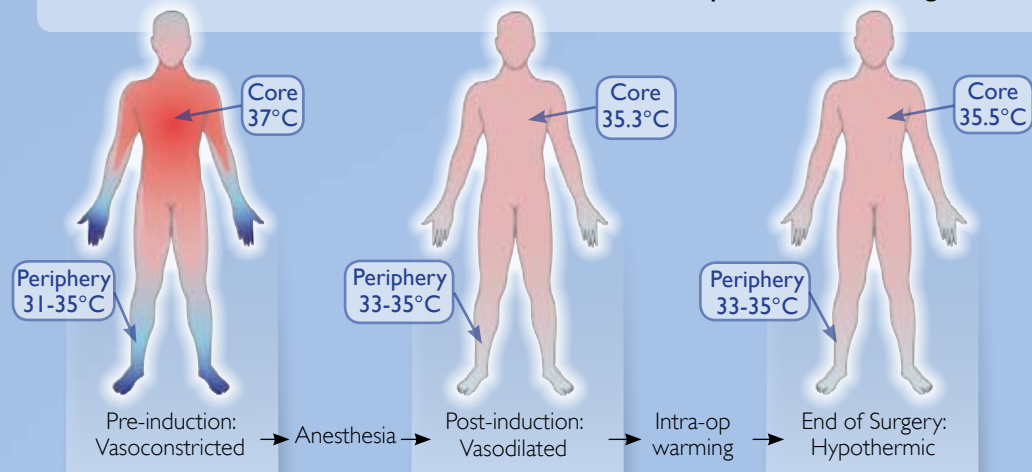

Anesthesia causes hypothermia

- Anesthesia causes vasodilation and a free flow of warm blood from the core to the cooler legs (periphery). This causes a rapid drop in core temperature—"redistribution hypothermia."

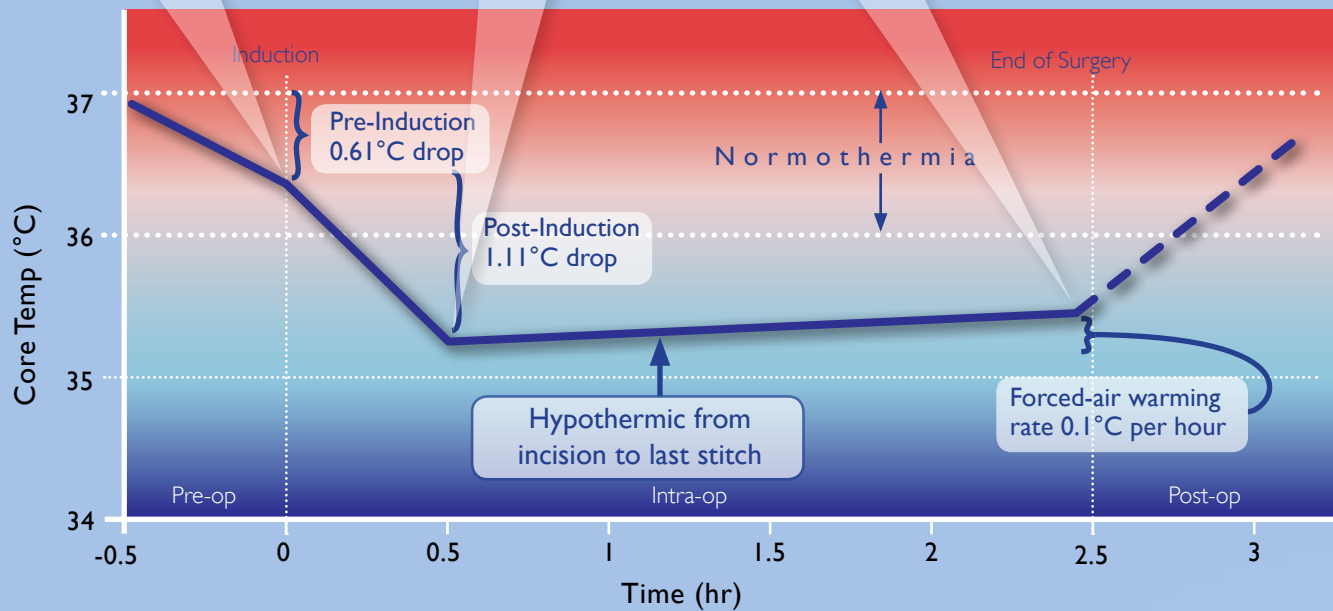

Intra-op forced-air warming cannot prevent redistribution hypothermia

- A review of 10 published studies reveals the average pre-induction temperature loss is 0.61°C¹⁻¹⁰ and the average post-induction redistribution temperature loss is 1.11°C⁶⁻¹³.
- Forced-air warming typically begins immediately following induction, but it does *nothing* to prevent the initial combined 1.72°C¹⁻¹³ drop in temperature. Most patients quickly become hypothermic after induction.


Forced-air warms only 0.1°C per hour

- The average of 10 published studies shows Bair Hugger® (forced-air warming) intraoperatively warms patients at **only 0.1°C per hour**.^{4-9,11,13-15}
- In a 2.5 hour surgery patients are frequently hypothermic from incision to the last stitch.
- Intraoperative warming with forced-air does not reliably prevent hypothermia, and it's also expensive.

Tomorrow's standard practice = Flatline™ normothermia


FLATLINE NORMOTHERMIA

Typical Pattern of Normothermia During General Anesthesia with Hot Dog® Flatline™ Warming

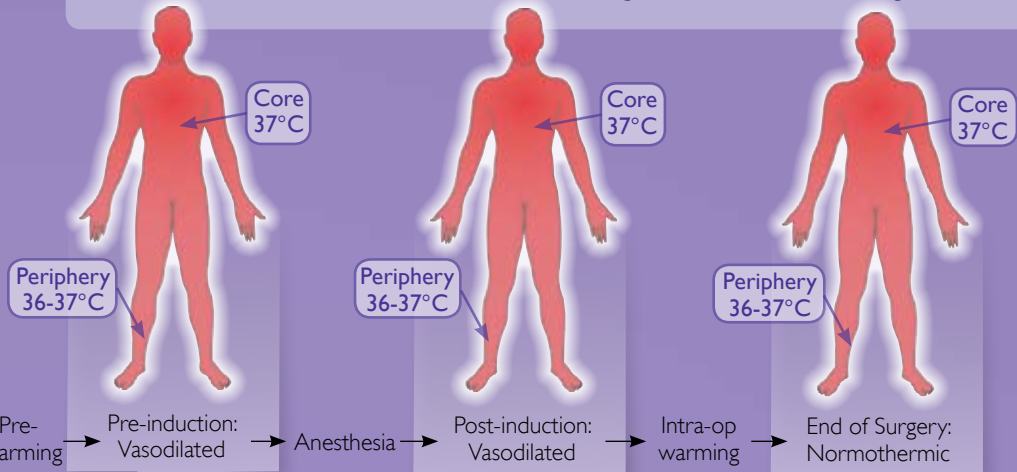

Pre-warming prevents hypothermia

- A continuum of warming throughout the perioperative process is necessary to prevent unintended hypothermia. Pre-warming the legs prior to induction is the *only* way to prevent the "redistribution hypothermia" resulting from anesthesia.

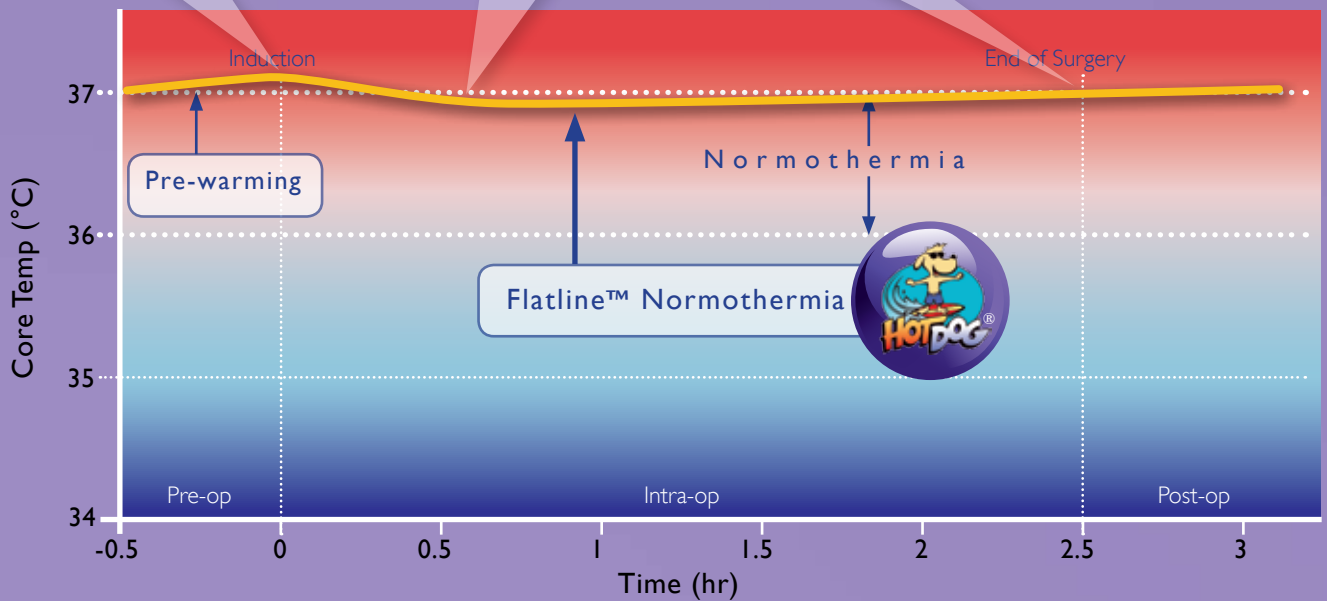

Pre-Op

Intra-Op


Post-Op



- Hot Dog® warming is designed to warm patients at every stage of the surgical process in a low-cost, highly effective manner.
- Continuing to warm the patient intraoperatively will maintain a normothermic body temperature throughout the case.
- The patient never becomes hypothermic and avoids the risks associated with hypothermia: increased wound infections, increased bleeding and increased morbid cardiac events.

Flatline™ Normothermia *and* Flatline Costs

Total Cost per Operating Room per Day

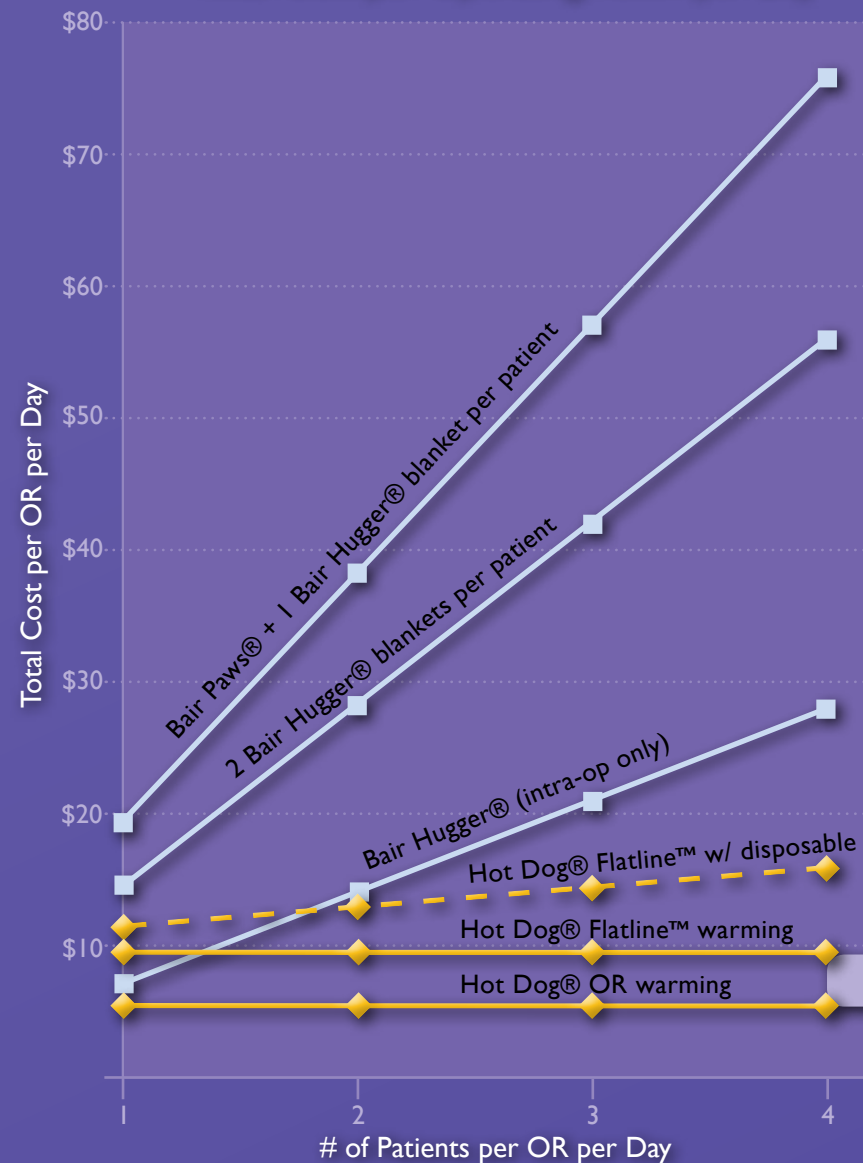

Normothermia isn't the only Flatline you'll get with Hot Dog®!

- Hot Dog warming provides Flatline normothermia for a Flatline cost of less than \$10 per day—that's \$10 total for all patients in that operating room that day!
- Even if yesterday's standard practice of only warming intra-op is your preference, try Hot Dog warming at around \$5.25 per OR per day!



Hot Dog® Flatline™
The NEXT WAVE in
Temperature Management
www.HotDogWarming.com

FLATLINE COST

Need yet another reason to go [air-free] in the operating room with Hot Dog?
Visit www.BlowingAirIsRisky.com to learn about the risks of blowing air in the OR.
Whats growing inside *your* hot-air blowers?

Hot Dog USA LLC
7536 Washington Ave. S.
Eden Prairie, MN 55344
Phone: 888-HD-Warms
(888-439-2767)
www.hotdog-usa.com



Hot Dog International LLC
6581 City West Parkway
Eden Prairie, MN, USA 55344
Phone: (952) 465-3500
Fax: (952) 465-3501
www.HotDogWarming.com

References ©2008 Hot Dog International, LLC. All Rights Reserved.

- 1.) Vanni SMD, et al. Preoperative combined with intraoperative skin-surface warming avoids hypothermia caused by general anesthesia and surgery. *J Clin Anesth.* 2003; 15:119-125.
- 2.) Chandon M, et al. Prevention of postoperative shivering by pre or intraoperative skin surface warming. *Anesthesiology.* 1994; 81:A561.
- 3.) Gauthier RL. Use of forced air warming system for intraoperative warming. *Anesthesiology.* 1990; 73:A462.
- 4.) Kabbara A, et al. Randomized prospective comparison of forced air warming using hospital blankets versus commercial blankets in surgical patients. *Anesthesiology.* 2002; 97:338-44.
- 5.) Smith, et al. Use of forced-air warming during and after outpatient arthroscopic surgery. *Anesth Analg.* 1994; 78:836-841.
- 6.) Negishi C, et al. Resistive-heating and forced air warming are comparably effective. *Anesth Analg.* 2003; 96:1683-7.
- 7.) Kurz A, et al. Perioperative normothermia to reduce the incidence of surgical-wound infection and shorten hospitalization. *NEJM.* 1996; 334:1209-1215.
- 8.) Borms SF, et al. Bair Hugger forced-air warming maintains normothermia more effectively than Thermo-Lite insulation. *J Clin Anesth.* 1994; 6:303-307.
- 9.) Camus Y, et al. Leg warming minimizes core hypothermia during abdominal surgery. *Anesth Analg.* 1993; 77:995-999.
- 10.) Just B, et al. Prevention of intraoperative hypothermia by preoperative skin-surface warming. *Anesthesiology.* 1993; 79:214-218.
- 11.) Hynson JM, et al. Intraoperative warming therapies: A comparison of three devices. *J Clin Anesth.* 1992; 4:194-199.
- 12.) Murat I, et al. Evaluation of the efficacy of a forced-air warmer (Bair Hugger) during spinal surgery in children. *J Clin Anesth.* 1994; 6:425-429.
- 13.) Matsukawa T, et al. Heat flow and distribution during induction of general anesthesia. *Anesthesiology.* 1995; 82:662-673.
- 14.) Bennett J, et al. Prevention of hypothermia during hip surgery: effect of passive compared with active skin warming. *Br J Anaesthesia.* 1994; 73:180-183.
- 15.) Kurz A, et al. Forced-air warming maintains intraoperative normothermia better than circulating-water mattresses. *Anesth Analg.* 1993; 77:89-95.

PN M102 Rev B

Not All Flatlines Are Bad.

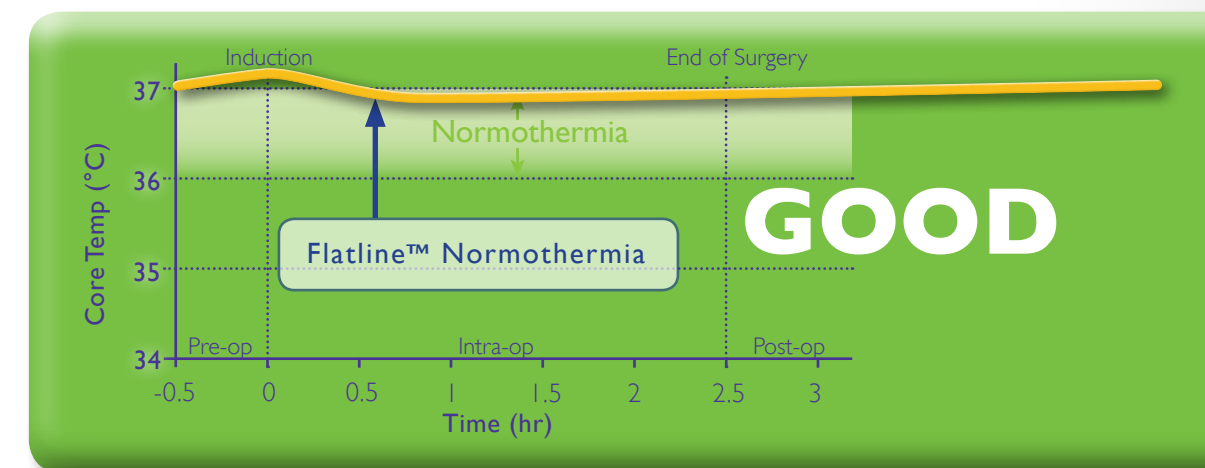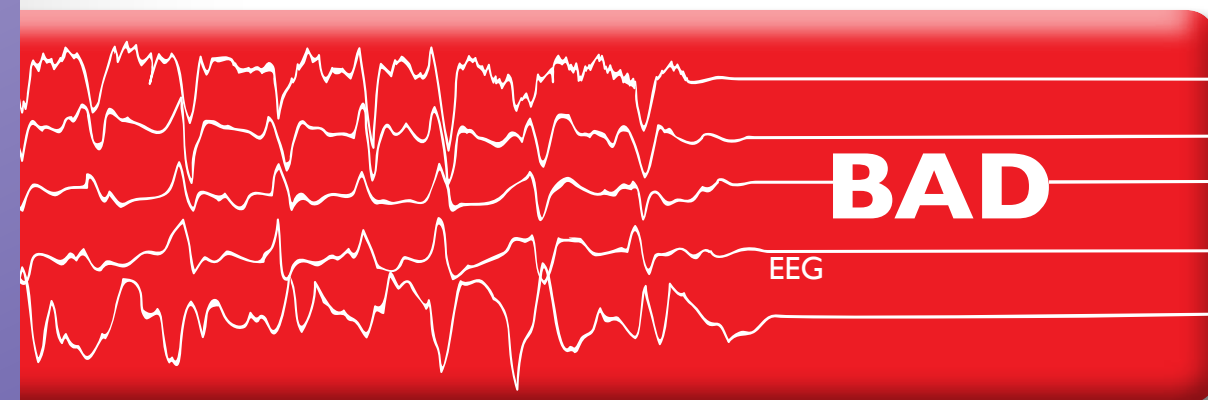

The NEXT WAVE in
Temperature Management:
Flatline™